

Lafayette Manual Muscle Test System User Instructions



P.O. Box 5729
Lafayette, IN 47903 USA
Tel: (765) 423-1505 • (800) 428-7545
Fax: (765) 423-4111
info@lafayetteinstrument.com
www.lafayetteinstrument.com

S.I. Instruments
256 South Rd. Hilton
South Australia 5033
Ph (08) 8352 5511

info@si-instruments.com.au
www.si-instruments.com.au

Table of Contents

Features	2
Specifications	3
Precautions	3
Basic Operations	3
Function Buttons	4
Screens	4
Resets	9
Accessories	10
Appendix A - Torque Measurements with the MMT	10
CE Declaration of Conformity	11

The Lafayette Manual Muscle Tester (MMT) System is an ergonomic hand-held device used for objectively quantifying muscle strength. The test is performed with the clinician applying force to the limb of a patient. The objective of the test is for the clinician to overcome or “break” the patient’s resistance. The MMT records the peak force and the time required to achieve the “break” providing reliable, accurate, and stable muscle strength readings.

The MMT also features interactive menus to allow a wide range of options such as data storage, preset test times, and force thresholds to be implemented. While powerful and versatile, the MMT is still small enough to fit comfortably in the palm of the hand. Its ergonomic design allows for both patient and tester comfort while easily conforming to manual muscle testing protocols.

Features

- Designed for high inter and intra instrument reproducibility
- Three, easy to change molded plastic stirrups with pads
- Force measurements in pounds, kilograms, or Newton (user selectable)
- Measures peak force, time to reach peak force, total test time, time within selectable ranges, and the average force
- Data storage for up to 150 tests in on-board memory
- Automatic or manual storage of data
- Measurement range 0-300lbs (136.1kg/1335N)
- Selectable test time form 1 – 10 seconds
- Tone to indicate start, stop, and entering within a range
- Microprocessor controlled
- Built-in stored data browsing capability
- Easy to read graphical LCD display
- Automatic shut off after 5 minutes of inactivity
- Battery indicator on LCD display
- Interactive menus allowing users to select device options
- Battery powered: (1) rechargeable lithium-ion battery
- Minimal measurement drift

Specifications

- Size: 3.16" x 5.11" x 1.6" (8.03cm x 12.98cm x 4.1cm)
- Weight: 312 g
- Range: 0-300 lbs (136.1kg) (1335 N)
- Accuracy: $\pm 1\%$ over full scale or ± 0.2 lbs
- Resolution: 0.1lbs/0.1kg/0.1N(0-999.9N) / 1N(1000N-1335N)
- Battery Life: 6 hrs powered on, 30 minutes after low battery condition
- Charge Time: 80% charge => 45 minutes / Full charge => 2 hrs
- Data Storage Capacity: 150 tests
- Preset Test Length: 0.5-10 seconds; in 0.1 second increments

Precautions

- When performing repeated tests, inconsistent placement of the MMT will adversely affect scores.
- Extreme temperature, especially heat, may affect the values obtained.
- The MMT cannot tolerate the stress of being used as a floor scale.
- Care should be taken not to drop the MMT, as it may affect the calibration.
- Exceeding the force limit (300lbs/136kg/1335N) may permanently damage and/or invalidate the calibration of the MMT.
- Upon initial receipt of MMT, charge for 2 hours.
- Stirrup should be rotated clockwise on and off to reduce friction on O-ring.

Basic Operations

The Lafayette MMT is small enough to be held in one hand and easily read. The size and weight of the MMT permit the examiner to use the same procedures and break test techniques described in the literature and taught by academic institutions without any modification of technique or positioning. The unit is simply placed between the examiner's hand and the limb being tested. The examiner's downward force is transmitted to the limb through the MMT unit. The MMT is designed for one hand operation. It can comfortably fit in the right or left hand, with settings for both dexterities. The hand is placed under the strap and around the body of the MMT. This allows easy access to the TOP buttons with the thumb. All of the other buttons are pressed using the opposite hand.

The MMT is activated by pressing the Menu/Select button. Measurements are taken by pressing the padded stirrup against the muscle being tested on the subject. The force and time data are displayed on the LCD screen. To conserve battery life, the MMT will deactivate itself when not in use for five minutes. All data on the main screen at power down is saved and will be shown when the MMT is activated again.

Function Buttons

The MMT has five function buttons that control the menus and allow the selection of options and settings.

1. **POWER/MENU/SELECT Button:** The round MENU/SELECT button is located on the bottom middle of the MMT. This is the button used to power on the device. Holding the MENU/SELECT button for 5 seconds will power off the unit. It is placed for easy access regardless of right or left hand operation. The MENU/SELECT allows you to enter into the Menu screen and select various options within it.
- 2, 3. **NAVIGATION Buttons:** While on the Test screen the NAVIGATION buttons are used to enlarge the graph and return back to the Test screen from the enlarged graph. While in the Menu screen, the NAVIGATION buttons are used to navigate the various menu screens.
- 4, 5. **TOP buttons:** On the Main screen the TOP buttons are used to SEND, CLEAR, and START tests when applicable. On the menu screen these buttons are used to return back one screen, BACK, or return to the Test screen, TEST. These buttons can be flipped for a specific dexterity by changing the button orientation in the OPTIONS menu.




Screens

Test Screen

The Main Measurement Screen shows all measurement information that is being captured. This screen is shown whenever a measurement is in progress. (see diagram on next page)

1. **Battery Indicator:** Indicates the remaining capacity in the charge of the battery.
2. **Force over Time Graph Area:** The graph displays the data for the previously conducted test, and automatically populates the chart to maximize the viewing area. The Y-axis label shows the amount of force (in lbs, kg, or N), and the X-axis shows the time in seconds.


3. Ave. Force: Average force exerted over the range.
4. Total Time: The total time is the total duration of the test in seconds.
5. Time-Peak: Time to peak is the elapsed time in seconds from the start of the test until the maximum force has been reached.
 - Each of these three windows can have any of the following measurements displayed during or after a test is taken:
 - *Real-Time Force*: This displays the real time force that is measured during the test.
 - *Time in Range*: Cumulative time within the specified range
 - *Time ↑ Range*: Cumulative time above the specified range
 - *Time ↓ Range*: Cumulative time below the specified range
6. Clear (Top Button Function): This area shows the current function for the top button. In the Test screen window, shown above, the clear function clears the current test, and allows the user to take another test.
7. Wireless Communication Indicator: This character indicates when the wireless is enabled.
8. Time Display: This time is displayed and can be set manually or synced with a PC in the Options Menu.
9. Sound Indicator: Indicates whether beeper is on or off for the current test.
10. Peak Force: The peak force displays the maximum force during the test and displays what units the force is being measured in (lbs, kg, or N).

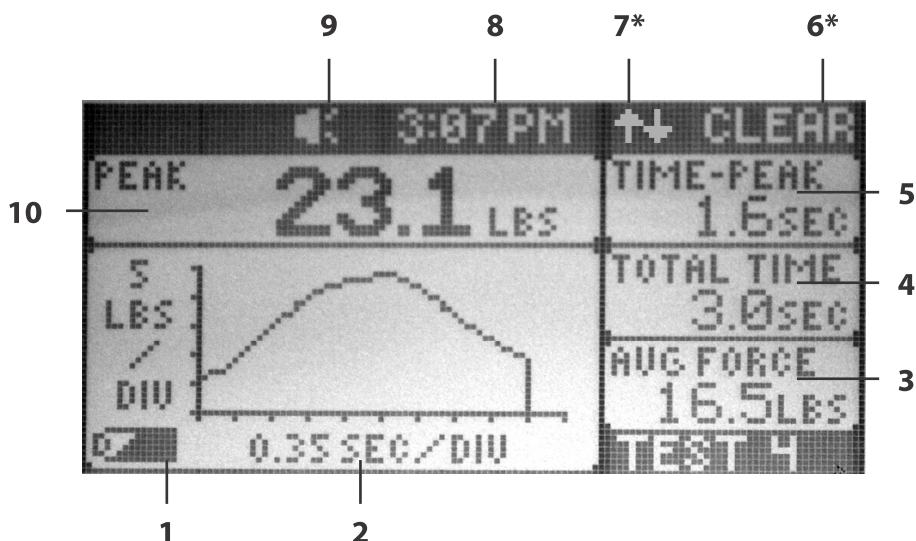

* indicates elements that will move depending on chosen button orientation - set in OPTIONS menu

Low Battery Indicator Screen & Charging

The low battery indicator screen is shown when the battery needs to be charged. The screen will appear and then the system will power off. This screen will re-appear when the power button is pressed until the unit is recharged via the USB connector. The device should take about 45 minutes to charge 80% of the capacity, or about 2 hours for a full charge.

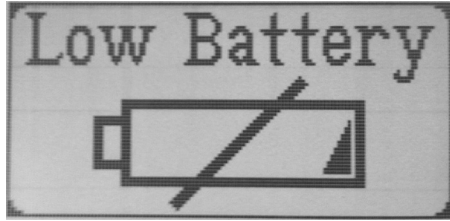

Test Setup Menu Screen

The Test Setup menu screen allows the user to setup various test options.

START

Starting a test can either be done by passing a FORCE THRESHOLD., or after a certain amount of TIME DELAY, triggered by the top button.

START FORCE/TIME DELAY

These options allow you to select customized force thresholds and time delays.

STOP THRESHOLD

If enabled, the test will end when the force applied drops below the value set in STOP FORCE. If disabled, the test will resume for the amount of time set by the TEST TIME.

STOP FORCE

If STOP THRESHOLD is enabled, each test will be stopped when the force is less than or equal to this force. Stop force cannot exceed start force.

AUTO CLEAR

If enabled, manually clearing the data is not required prior to starting new tests.

UNITS

Allows selection of pounds (lbs), kilograms (kg), or Newtons (N).

TEST TIME




Allows users to select preset time for testing.

RANGE

Allows an upper and lower range to be enabled for testing. These ranges are set by setting the UPPER RANGE and LOWER RANGE.

RANGE TONES (↑ RANGE TONE, IN RANGE TONE, ↓ RANGE TONE)

Range tones are enabled by turning on each corresponding tone. The ↑ RANGE TONE is a single beep. The IN RANGE TONE is two quick beeps. The ↓ RANGE TONE is three quick beeps.

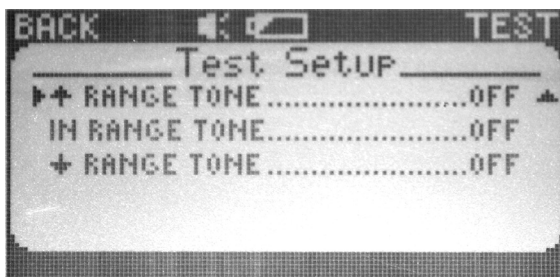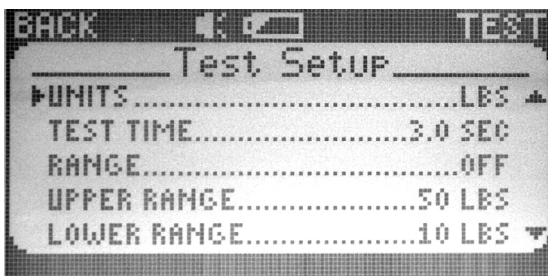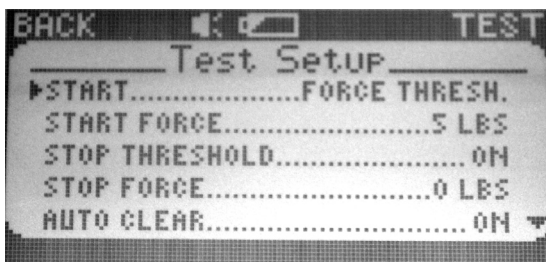

Saved Data Menu Screen

The Saved Data menu screen allows users to manage tests that have been saved in the internal memory.



TEST	PEAK	T-PEAK	TOTAL-T
10	23.0LBS	2.3SEC	2.8SEC
09	23.2LBS	1.6SEC	10.0SEC
08	23.1LBS	0.7SEC	10.0SEC
07	8.6LBS	1.4SEC	10.0SEC

TEST	PEAK	T-PEAK	TOTAL-T
10	23.0LBS	2.3SEC	2.8SEC
09	23.2LBS	1.6SEC	10.0SEC
08	23.1LBS	0.7SEC	10.0SEC
07	8.6LBS	1.4SEC	10.0SEC

Options Menu Screen

The Options menu allows user to customize the setup of their unit.

WIRELESS

Toggles on/off the module for wireless connection.

DISPLAYS 1, 2, 3

Correspond to the customizable measurement areas on the Test Screen

BUTTON ORIENTATION

Switches the functionality of the top buttons, allowing for use in either hand.

BACKLIGHT

Toggles unit's backlight on/off.

SOUND

Toggles unit's sound on/off.

PC TIME SYNC


Allows the MMT to automatically set its time when connected to a PC

DATE

Updates the MMT system date.

TIME

Updates the MMT system time.

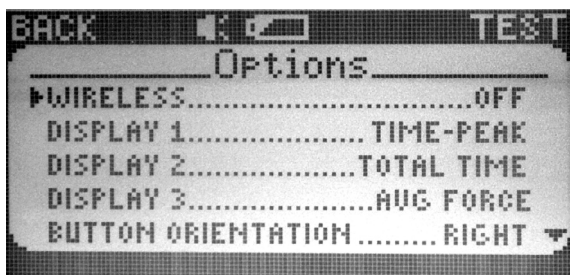

Information Menu Screen

The Information menu screen provides a contact email and various information about the MMT.



Resets

To restore MMT to factory defaults, press MENU/SELECT and navigate to the Information screen. Press and hold MENU/SELECT then press the upper left button until screen reads "Restored Defaults".

Hard Reset: If the MMT freezes press MENU/SELECT and the upper right button until the unit powers off.

S.I. Instruments
256 South Rd. Hilton
South Australia 5033
Ph (08) 8352 5511

info@si-instruments.com.au
www.si-instruments.com.au

Accessories



Disposable Sanitary Covers

Model 01165SC

Replacement Set of 25 adhesive Sanitary Covers for MMT Stirrups.



MMT Replacement Kit

Model 01165RK

Replacement Set of Stirrups, O-rings, and Sanitary Covers for the MMT.

Appendix A – Torque measurements with the MMT

In some research and rehabilitation applications, it is necessary to obtain torque measurements for the limb being tested. Torque is often a more accurate indicator of total strength because it takes into account the length of the muscle being tested. The Lafayette Manual Muscle Test System (MMT) can be used to obtain torque values through a series of basic calculations.

Torque is measured in units of Newton meters (Nwm) in the Metric system and in foot pounds (ftwlbs) in the English system. Torque is the product of the force applied times the distance between the force and the pivot point (usually a joint).

Equations for obtaining torque readings with the MMT using metric values:

$$\text{Torque} = \text{Force} * \text{Distance}$$

Where force equals the MMT reading converted to Newtons and distance is the length between where the force is applied and the joint being tested in meters.

Newtons conversions: 1 pound = 4.45 Newtons; 1 kilogram = 9.81 Newtons
Newtons are calculated at sea level.

Normative Strength can also be quantified as torque per kilogram bodyweight (Nwm/kg). This value is obtained by dividing the torque by the person's bodyweight in kg.

$$\text{Strength} = \frac{((\text{MMT reading in Newtons}) * \text{distance})}{\text{bodyweight in kilograms}}$$

CE - DECLARATION OF CONFORMITY

The following apparatus:

Product Name: Manual Muscle Tester
Model Designation: 01165

Manufacturer's Name: Lafayette Instrument Company
Manufacturer's Address: 3700 Sagamore Parkway North
 Lafayette, Indiana 47904
 U.S.A.

is hereby confirmed to comply with the essential requirements set out in the Medical Device Directive 2007/47/EC and the Electromagnetic Compatibility Directive 2004/108/EC. This product is a Class I Medical Device requiring self-certification only. For the evaluation regarding the electromagnetic compatibility requirements, the following standards were applied:

Electromagnetic Compatibility	Electrical Safety
IEC 60601-1-2 :2007-03	IEC 60601-1-1 :2000
CISPR 11	
IEC 61000-4-2	
IEC 61000-4-3	
IEC 61000-4-8	

The following manufacturer/importer is responsible for this declaration:

Company Name: Lafayette Instrument Company
Company Address: 3700 Sagamore Parkway North
 Lafayette, Indiana 47904
 U.S.A.

Person responsible for making this declaration:

Name: Brent E. Smitley
Position/Title: Engineering Manager
Place: Lafayette, Indiana U.S.A.

Legal Signature:



Terms and Conditions

LIC Worldwide Headquarters

Toll-Free: (800) 428-7545 (USA only)

Phone: (765) 423-1505

Fax: (765) 423-4111

Email: sales@lafayetteinstrument.com

export@lafayetteinstrument.com (Outside the USA)

Mailing Address:

Lafayette Instrument Company

PO Box 5729

Lafayette, IN 47903, USA

Lafayette Instrument Europe:

Phone: +44 1509 817700

Fax: +44 1509 817701

Email: eusales@lafayetteinstrument.com

Phone, Fax, Email or Mail-in Orders

All orders need to be accompanied by a hard copy of your purchase order. All orders must include the following information:

- Quantity
- Part Number
- Description
- Your purchase order number or method of pre-payment
- Your tax status (include tax-exempt numbers)
- Shipping address for this order
- Billing address for the invoice we'll mail when this order is shipped
- Signature and typed name of person authorized to order these products
- Your telephone number
- Your email address
- Your FAX number

Domestic Terms

There is a \$50 minimum order. Open accounts can be extended to most recognized businesses. Net amount due 30 days from the date of shipment unless otherwise specified by us. Enclose payment with the order; charge with VISA, MasterCard, American Express, or pay COD. We must have a hard copy of your purchase order by mail, E-mail or fax. Students, individuals and private companies may call for a credit application.

International Payment Information

There is a \$50 minimum order. Payment must be made in advance by: draft drawn on a major US bank; wire transfers to our account; charge with VISA, MasterCard, American Express, or confirmed irrevocable letter of credit. Proforma invoices will be provided upon request.

Exports

If ordering instrumentation for use outside the USA, please specify the country of ultimate destination, as well as the power requirements (110V/60Hz or 220V/50Hz). Some model numbers for 220V/50Hz will have a "C" suffix.

Quotations

Quotations are supplied upon request. Written quotations will include the price of goods, cost of shipping and handling, if requested, and estimated delivery time frame. Quotations are good for 30 days, unless otherwise noted. Following that time, prices are subject to change and will be re-quoted at your request.

Cancellations

Orders for custom products, custom assemblies or instruments built to customer specifications will be subject to a cancellation penalty of 100%. Payment for up to 100% of the invoice value of custom products may be required in advance. Cancellation for a standard Lafayette Instrument manufactured product once the product has been shipped will normally be assessed a charge of 25% of the invoice value, plus shipping charges. Resell items, like custom products, will be subject to a cancellation penalty of 100%.

Exchanges and Refunds

Please see the cancellation penalty as described above. No item may be returned without prior authorization of Lafayette Instrument Company and a completed Return Form. A copy of the Return Form or your assigned Return # (you will receive this via email after submitting the form) must be included with the returned goods. The merchandise should be packed well and fully insured. Unopened merchandise may be returned prepaid within thirty (30) days after receipt of the item and in the original shipping carton. Collect shipments will not be accepted. Returned products must be in saleable condition, and credit is subject to inspection of the merchandise.

Repairs

Instrumentation may not be returned without prior authorization by Lafayette Instrument Company and a completed Return Form. When you

complete the Form, or call Lafayette Instrument, you will receive a Return #. Your Return # number will be good for 30 days. Address the shipment to:

Lafayette Instrument Company

3700 Sagamore Parkway North

Lafayette, IN 47904, USA.

Shipments cannot be received at the LIC PO Box. Items should be packed well, insured for full value, and returned along with a copy of the Return Form or the Return #. An estimate of repair will be given prior to completion ONLY if requested in an enclosed cover letter. We must have a completed purchase order by mail or fax, or repair work cannot commence for non-warranty repairs.

Damaged Goods

Damaged instrumentation should not be returned to Lafayette Instrument prior to a thorough inspection. If a shipment arrives damaged, note damage on delivery bill and have the driver sign it to acknowledge the damage. Contact the delivery service, and they will file an insurance claim. If damage is not detected at the time of delivery, contact the carrier/shipper and request an inspection within 10 days of the original delivery. Please call the Lafayette Instrument Customer Service Department for repair or replacement of the damaged merchandise.

Limited Warranty

Lafayette Instrument Company warrants equipment manufactured by the company to be free of defects in material and workmanship for a period of one year from the date of shipment, except as provided hereinafter. The original manufacturer's warranty will be honored by Lafayette Instrument for items not manufactured by Lafayette Instrument Company, i.e. resell items. This assumes normal usage under commonly accepted operating parameters and excludes consumable products.

Warranty period for repairs or used instrumentation purchased from Lafayette Instrument is 90 days. Lafayette Instrument Company agrees either to repair or replace, at its sole option and free of part charges to the customer, instrumentation which, under proper and normal conditions of use, proves to be defective within the warranty period. Warranty for any parts of such repaired or replaced instrumentation shall be covered under the same limited warranty and shall have a warranty period of 90 days from the date of shipment or the remainder of the original warranty period whichever is greater. This warranty and remedy are given expressly and in lieu of all other warranties, expressed or implied, of merchantability or fitness for a particular purpose and constitutes the only warranty made by Lafayette Instrument Company.

Lafayette Instrument Company neither assumes nor authorizes any person to assume for it any other liability in connection with the sale, installation, service or use of its instrumentation. Lafayette Instrument Company shall have no liability whatsoever for special, consequential, or punitive damages of any kind from any cause arising out of the sale, installation, service or use of its instrumentation. All products manufactured by Lafayette Instrument Company are tested and inspected prior to shipment. Upon prompt notification by the Customer, Lafayette Instrument Company will correct any defect in warranted equipment of its manufacture either, at its option, by return of the item to the factory, or shipment of a repaired or replacement part. Lafayette Instrument Company will not be obliged, however, to replace or repair any piece of equipment, which has been abused, improperly installed, altered, damaged, or repaired by others. Defects in equipment do not include decomposition, wear, or damage by chemical action or corrosion, or damage incurred during shipment.

Limited Obligations Covered by this Warranty

1. In the case of instruments not of Lafayette Instrument Company manufacture, the original manufacturer's warranty applies.
2. Shipping charges under warranty are covered only in one direction. The customer is responsible for shipping charges to the factory if return of the part is required.
3. This warranty does not cover damage to components due to improper installation by the customer.
4. Consumable and/or expendable items, including but not limited to electrodes, lights, batteries, fuses, O-rings, gaskets, and tubing, are excluded from warranty.
5. Failure by the customer to perform normal and reasonable maintenance on instruments will void warranty claims.
6. If the original invoice for the instrument is issued to a company that is not the company of the end user, and not an authorized Lafayette Instrument Company distributor, then all requests for warranty must be processed through the company that sold the product to the end user, and not directly to Lafayette Instrument Company.

Export License

The U.S. Department of Commerce requires an export license for any polygraph system shipment with an ULTIMATE destination other than: Australia, Japan, New Zealand or any NATO Member Countries. It is against U.S. law to ship a Polygraph system to any other country without an export license. If the ultimate destination is not one of the above listed countries, contact us for the required license application forms.